



Calibration Report

Report Number: 20250821-1253281

221 East Lincoln Avenue, Fort Collins, CO 80524 USA
1-970-498-1500, 1-800-446-7488, FAX: 1-970-498-1598

Visit us at www.in-situ.com

Instrument Details:

Instrument Model: Level TROLL 500
Full Scale Pressure Range: 5 PSI / 3.5 m / 11.5 ft / vented
Serial Number: 1253281
Hardware Version: 7
Firmware Version: 3.1

L13-1

Calibration Details:

Calibration Result: PASS
Calibration Date: 2025-08-21 15:52:04 (UTC)
Nominal Range of Applied Temperature: -5 C to +50 C
Temperature Accuracy Specification: +/- 0.1 C From -5 C to +50 C
Nominal Range of Applied Pressure: 0 PSI to 5 PSI
Pressure Accuracy Specification: +/- 0.05% FS From -5 C to +50 C

Post-Calibration Check:

Parameter	Applied	Reported	Deviation	Unit
Pressure	5.0000	5.0007	0.0007	PSI
Pressure	2.0000	1.9998	-0.0002	PSI
Pressure	-0.0002	0.0004	0.0005	PSI
Temperature	40.1980	40.2067	0.0087	C

Calibration Procedures and Equipment Used:

Automated calibration procedures used.

Manu Agilent Model 34970A SerialNo US37022274

Manu Mensor Model CPC6050 SerialNo 41001x3P

Manu Instrulab Model 3312A-14-15-24 SerialNo 31102


Manu Instrulab Model 406X-0031-01 SerialNo 21663-2

Manu Agilent Model 53131A-010 SerialNo MY47002282

Manu MENSOR Model 600 SerialNo 620699

Notes:

- Standards used in this calibration are traceable to the National Institute of Standards and Technology.
- This calibration report shall not be reproduced, except in full, without the written approval of In-Situ, Inc.
- A calibration interval of 12 to 18 months is recommended.

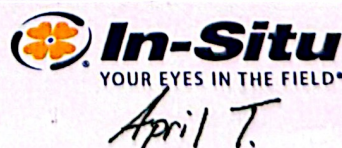

Performed By: TG

Report generated 8/27/2025 8:23:43 PM

Copyright © 2005-2025 In-Situ, Inc.

Page 1 of 1